



Surface enhanced Raman spectroscopybased detection of drug permeation in an intestinal cell model

Viehrig, Marlitt; Zor, Kinga; Rindzevicius, Tomas; Schmidt, Michael S.; Müllertz, Annette ; Boisen, Anja

Publication date:
2018

Document Version
Publisher's PDF, also known as Version of record

[Link back to DTU Orbit](#)

Citation (APA):
Viehrig, M., Zor, K., Rindzevicius, T., Schmidt, M. S., Müllertz, A., & Boisen, A. (2018). *Surface enhanced Raman spectroscopybased detection of drug permeation in an intestinal cell model*. Poster session presented at Biosensors 2018, Miami, Florida, United States.

General rights

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

Surface enhanced Raman spectroscopy-based detection of drug permeation in an intestinal cell model

Marlitt Viehri¹, Kinga Zór¹, Tomas Rindzevicius¹, Michael S. Schmidt¹, Annette Müllertz^{1,2}, Anja Boisen¹

¹The Danish National Research Foundation and Villum Foundation's Center for Intelligent Drug Delivery and Sensing Using Microcontainers and Nanomechanics (IDUN), Department of Micro- and Nanotechnology, Technical University of Denmark, Kgs. Lyngby, Denmark.


²Department of Pharmacy, University of Copenhagen, Copenhagen, Denmark.

We present the development of a detection strategy based on surface-enhanced Raman spectroscopy (SERS) sensing in liquids, relevant for biological samples. The SERS substrates, fabricated from free-standing, gold-capped silicon nanopillars are commonly used for the detection of analytes dissolved in organic solvents and dried on the sensor surface. We developed a method where detection can be performed directly in liquid using a model drug acetaminophene (Paracetamol).

SERS sensing in Cell Models

Intestinal Cell Model - Transwell® Systems


Caco-2 cells, are widely used as *in vitro* intestinal model. [2] Transwell® systems are used in *in vitro* drug permeation studies, where drugs are added to the transport media (e.g. Hanks' balanced salt solution (HBSS)).

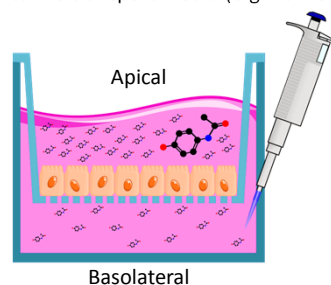


Samples are commonly analyzed with robust, but time and resource consuming techniques such as high-performance liquid chromatography. (Bio)sensors based on SERS offer fast, accurate and cost effective alternatives for identifying drug types and concentrations in permeation studies.

SERS Substrates – Gold Capped Nanopillars

SERS is a powerful analysis technique capable of detecting molecular fingerprints of analytes with high sensitivity and fast response time. [3]




Classical dry droplet SERS sensing using gold-capped Si nanopillars. [4]




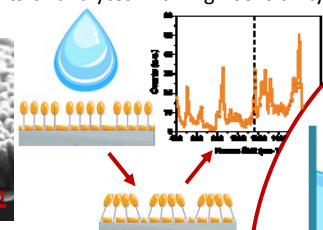


Droplet SERS

Dry droplet SERS-based detection of paracetamol.




Dry droplet measurements are highly influenced by solvent composition. Complex matrices like HBSS can lead to fouling of the sensors. To enable droplet measurements it was necessary to dilute HBSS 1:10 with pure ethanol.



Paracetamol spiked in pure ethanol and HBSS. Calibration curves were obtained following the characteristic paracetamol peak at 1160 cm⁻¹. We found that Paracetamol dissolved in ethanol can be detected in a linear range between 35 – 200 μM, while when spiked in HBSS and diluted 1:10 with EtOH a linear trend between 50 – 350 μM is observed.


Surface Treatment

UV/ ozone exposure is commonly utilized as surface treatment and cleaning procedure in a variety of microfabrication processes. It renders the surface of gold-capped nanopillars from hydrophobic to hydrophilic without any morphological alterations.


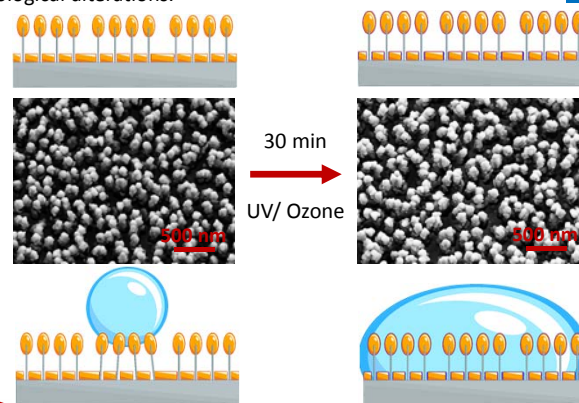


Liquid Measurements



UV/ ozone treatment enabled the development of a novel liquid measurement technique for nanopillar SERS based sensing.

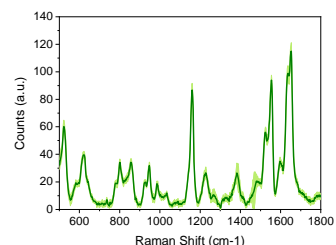

Detection of 350 μM paracetamol in liquid UV/ Ozone treated samples.



Paracetamol spiked in MQ and HBSS. Liquid detection of paracetamol in MQ is possible over a linear range of 5–100 μM. Direct liquid measurements in HBSS displayed a linear trend between 5 – 75 μM.



Acknowledgement

This work was financially supported by the IDUN Center of Excellence funded by the Danish National Research Foundation (Grant No. DNRF122) and the Villum Fonden (Grant No. 9301).

References

- [1] H. Lennernaes, "Regional intestinal drug permeation: biopharmaceuticals and drug development" in European Journal of Pharmaceutical Science, 2014, pp. 57:333–41.
- [2] C. Pereira, J. Costa, B. Sarmiento, and F. Araujo, "Cell-based *in vitro* models for intestinal permeability studies." in Concepts and Models for Drug Permeability Studies, Cell and tissue based *in vitro* culture models, 2016, pp. 57–81.
- [3] G. C. Schatz, M. A. Young, and R. P. Duyne, "Electromagnetic Mechanism of SERS," in Surface-Enhanced Raman Scattering, Springer Berlin Heidelberg, 2006, pp. 19–45.
- [4] M. S. Schmidt, J. Hübner, and A. Boisen, "Large Area Fabrication of Leaning Silicon Nanopillars for Surface Enhanced Raman Spectroscopy," Adv. Mater., vol. 24, no. 10, p. OP11-OP18, Mar. 2012.

